

TriA-SNOM Microscope

The invention and subsequent development of scanning probe microscopy (SPM) methods have produced the necessary tools for a step forward in optical measurements.





The possibility to go beyond the Abbe diffraction limit has been achieved with the Near-field light optical microscopes (SNOM). They employ SPMs precision of piezoelectric raster-scanning together with sharp probes to obtain light optical images at subwavelength resolution.

Particular care has been taken to different applications from solid state to biomedicine.

The goal of our company is to give to the customers the instrument that best fit their needs.

This product is the result of a collaboration between A.P.E. Research and National Research centers.

TriA-SNOM

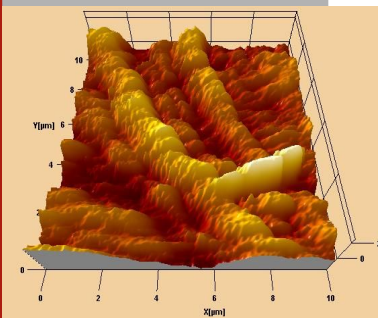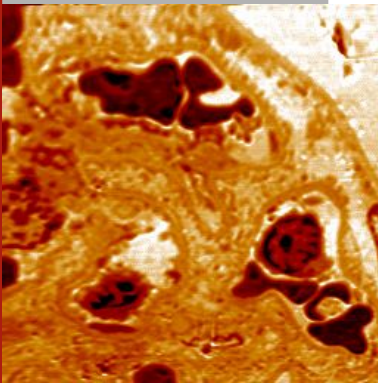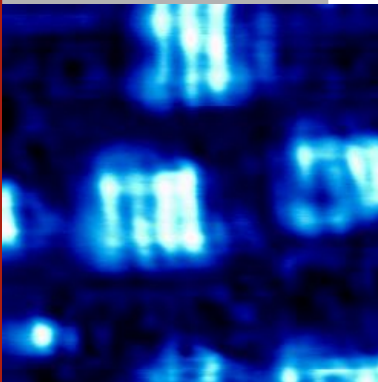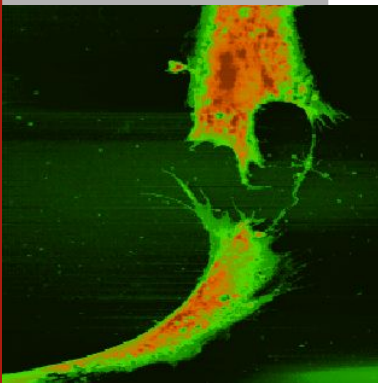

A100-SGS SPM Stage

Scanning stage with absolute positioning system with strain gauge sensors.

Scanner technical data:

X-Y scan size: 100 x 100 μm (high voltage mode);
10 x 10 μm (low voltage mode)
Resolution high voltage mode: Closed loop: 2 nm,
Open loop: 0.2 nm
Closed loop linearity: 0.1%.
Z scan size: 10 μm (high voltage mode)
1 μm (low voltage mode)
Resolution: 0.16 nm (high voltage mode),
0.02 nm (low voltage mode).

TriA-SNOM Head

SNOM Head is suitable for Simultaneous Acquisition of Optical signal (up to 3: reflection, transmission and collection mode) and Topographic signal.

Optical signals acquisition by 2 Photomultipliers.

Sample holder size: 30x30 mm;

Translator range 13 x 13 x 13 mm; servo assisted z movement.

2 Optical Vision System integrated into the SNOM head:

-Optical vision system to monitor probe approaching on the sample;

-Inverted optical microscope for Transparent sample.

A.P.E. Research suggests "Lovalite" SNOM probes.

Probe Holder is suitable for any Commercial SNOM fibers.

Dual demodulator

A.P.E. Research Dual demodulator for Optical signals acquisition.

SPMCU2-PI

SPM Control Unit

SPM Control Unit and PC (equipped with a multi input-output board) drives the scanner, data acquisition and sample motion.

Tip to sample distance is controlled by ultra-low noise analog feedback, digitally driven by PC.

HVA3-PI Unit

High Voltage Amplifier

HVA is an amplifier module projected to drive TriA-SNOM Heads.

Computer and Acq. Board

Windows XP/Vista operating system; Pentium Core 2 Duo, 1GB/2GB DDR2 SDRAM, 160 GB HDD, CD R/RW, mouse, keyboard; 17 inch LCD monitor. Acquisition board and interface.

Acquisition software

Software runs under Windows and is composed of a multi-window applications for instrument control and data acquisition. The software comes equipped with simple filters for immediate analysis of acquired images.

Accessories

Acoustic Box with floating marble

Table

Image Metrology SPIP™ data analysis software

Characteristics and technical specifications subject to change

A.P.E. Research s.r.l.
Area Science Park
s.s. 14, Km 163,5 Basovizza
I-34012 Trieste, Italy

Tel. +39.040.3757905
Fax +39.040.3757906
infos@aperesearch.com
www.aperesearch.com